


FLURIDONE DETAILED FLOWCHART

1.




Remove upper rack from magnetic base. Label test tubes for Standards, Control, and Samples.

Tube #	Content
1, 2	Diluent/Zero Standard 0 ppb
3, 4	Standard 1, 0.5 ppb
5, 6	Standard 2, 2.0 ppb
7, 8	Standard 3, 7.5 ppb
9, 10	Standard 4, 15.0 ppb
11, 12	Control
13, 14	Sample 1
15, 16	Sample 2
17, 18	Sample 3




Add 150 μ L of Standards, Control or Samples to the bottom of each test tube by inserting the pipette tip all the way into the bottom of the tube without touching the sides of the tube.

6.



Do not separate upper rack from lower base. Using a smooth motion, invert the combined rack assembly over a sink and pour out the tube contents; keep inverted and **gently blot** the test tube rims on several layers of paper toweling.

7.

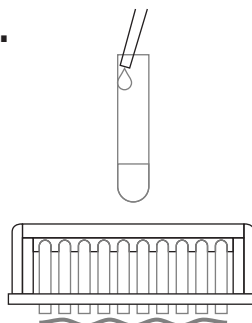


Add 1 mL of Washing Solution down the inside wall of each tube by using the technique described in Box 2. Wait 2 minutes. Using a smooth motion, invert the combined rack assembly over a sink and pour out the tube contents. Keep inverted and **gently blot** the test tube rims on several layers of paper toweling. Repeat this step 2 additional times.

2.



Add 250 μ L of Fluridone Enzyme Conjugate down the inside wall of each tube by aiming the pipet tip 1/4" to 1/2" below the tube rim without touching the rim or tube wall with the pipet tip; deliver liquid gently. *Vortex* for 1 to 2 seconds (at low speed to minimize foaming).

8.



Lift the upper rack (with its tubes) off the magnetic base; add 500 μ L of Color Solution down the inside wall of each tube by using the technique described in Box 2. *Vortex* for 1 to 2 seconds (at low speed to minimize foaming).

3.



Mix and Add 500 μ L of the thoroughly mixed Fluridone Antibody Coupled Paramagnetic Particles down the inside wall of each tube by aiming the pipet tip 1/4" to 1/2" below the tube rim without touching the rim or tube wall with the pipet tip; deliver liquid gently. *Vortex* for 1 to 2 seconds (at low speed to minimize foaming).

9.




React for 20 minutes at room Temperature (15°- 30° C). During this period, add 1 mL of Washing Solution into a clean tube for use as an instrument blank in Step 10.

4.



React 20 minutes at room temperature (15°- 30°C).

10.

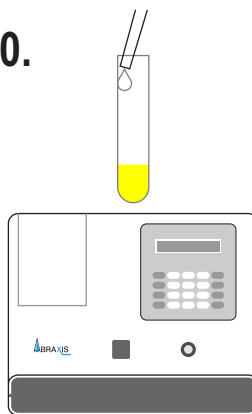

Add 500 μ L of Stopping Solution down the inside wall of each tube by using the technique previously described. Read results at 450 nm within 15 minutes after adding the Stopping Solution. Multiply results of samples by the appropriate dilution factor (if any).

[**Safety Caution:** Stopping Solution contains diluted sulfuric acid.]

For Ordering or Technical Assistance Contact:
ABRAXIS, LLC 54 Steamwhistle Drive, Warminster, PA 18974
Phone: 215-357-3911 Fax: 215-357-5232
Web: www.abraxiskits.com

Fluridone Magnetic Particle Kit Part # 500511, 100 Test




FLURIDONE CONCISE FLOWCHART

1.




Separate the rack.

Add 150 μ L of Standards, Control or Samples to the bottom of each test tube.



6.



Invert the combined rack to decant.

Blot **gently**.

7.




Add 1 mL of Washing Solution to each tube.

Wait 2 minutes.

Invert the combined rack to decant.

Blot **gently**.




2.



Add 250 μ L of mixed Fluridone Enzyme Conjugate to each test tube.

Vortex.

8.



Separate the rack.

Add 500 μ L of Color Solution to each test tube.

Vortex.



3.



Add 500 μ L of thoroughly mixed Magnetic Particles to each test tube.

Vortex.

9.



Incubate for 20 minutes.

Prepare blank.

4.




Incubate for 20 minutes.

10.




Add 500 μ L of Stopping Solution to each test tube.

Read OD 450



5.



Combine the rack and magnetic base.

Seat all tubes.

Wait 2 minutes.

For Ordering or Technical Assistance Contact:
ABRAXIS, LLC 54 Steamwhistle Drive, Warminster, PA 18974
Phone: 215-357-3911 Fax: 215-357-5232
Web: www.abraxiskits.com

Fluridone Magnetic Particle Kit Part # 500511, 100 Test